SRA INSTRUMENTS
CHROMATOGRAPHIC SOLUTIONS

APPLICATION NOTE AA0410-002

ON-SITE ANALYSIS OF ORGANOCHLORIDES AT TRACE LEVEL

Technique : µ-TD / µ-GC with battery

Sampling conditions with µ-TD :
TENAX TA 150 mg ; 60 seconds ; 100 mL.min $^{-1}$; 40°C

Desorption temperature : 190°C

Column : OV-1
Column temperature : 50°C
Column pressure : 25 psi

Carrier gas : Helium
Injector temperature : 80°C
Injection time : 100 ms

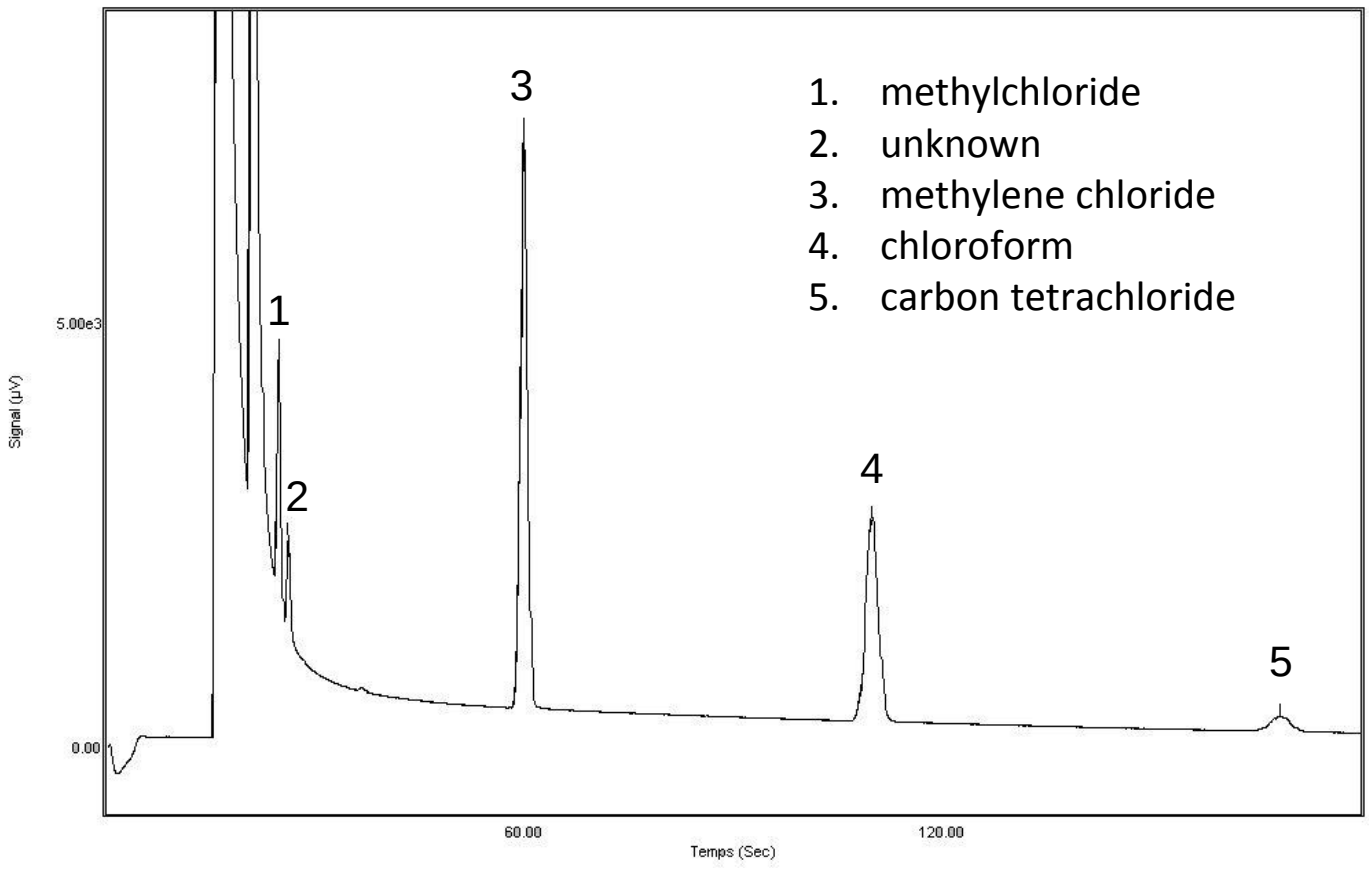

SRA INSTRUMENTS
210 rue des sources - 69280 Marcy l'Etoile - FRANCE
T +33 (0)4 78 44 29 47 - F +33 (0)4 78 44 29 62